


DIAGNOSTIC CHART

BEFORE MIXING: Fill 2 mL sterile empty vials with 1.8 mL diluent.

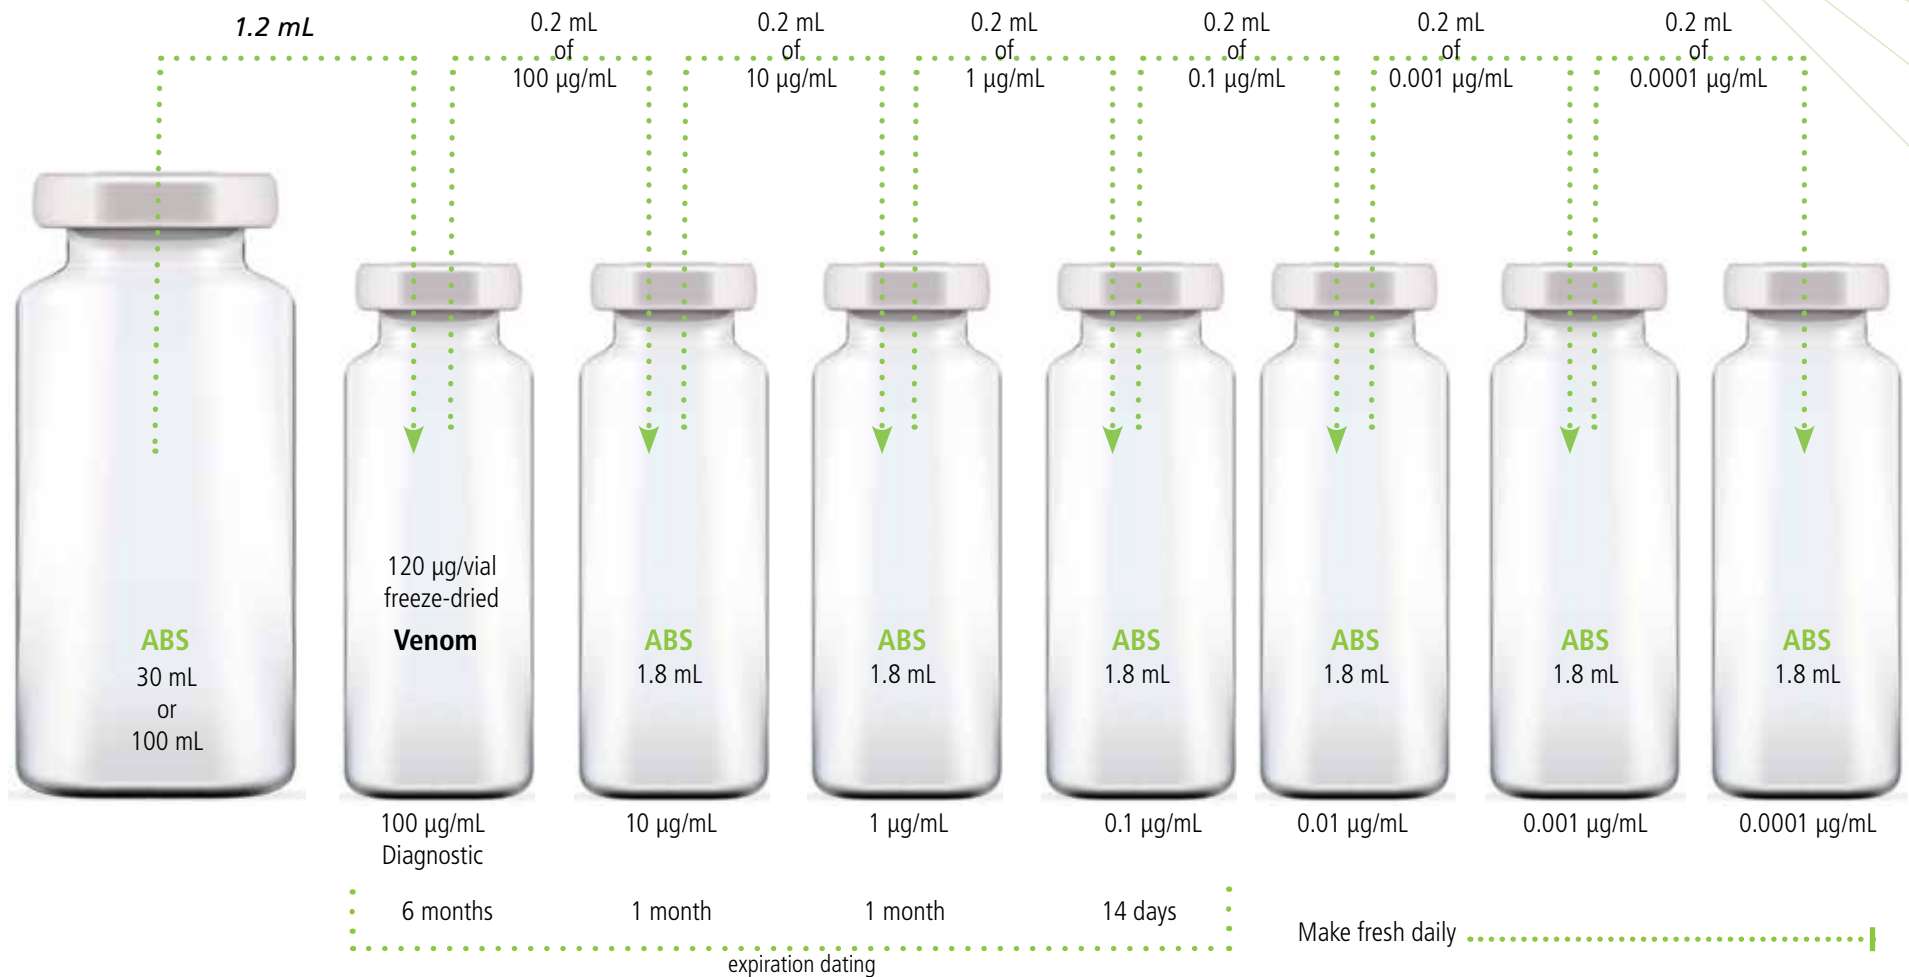

Vials not actual size.
For use with HollisterStier Allergy venom products only.
Always consult package insert for mixing instructions.

MAINTENANCE CHART



Expiration dating is 6 months after mixing

¹Mixed vespid venom protein concentrations will be 3x stronger

Vials not actual size.
For use with HollisterStier Allergy venom products only.
Always consult package insert for mixing instructions.