



BEFORE MIXING: Fill 2 mL sterile empty vials with 1.8 mL diluent.

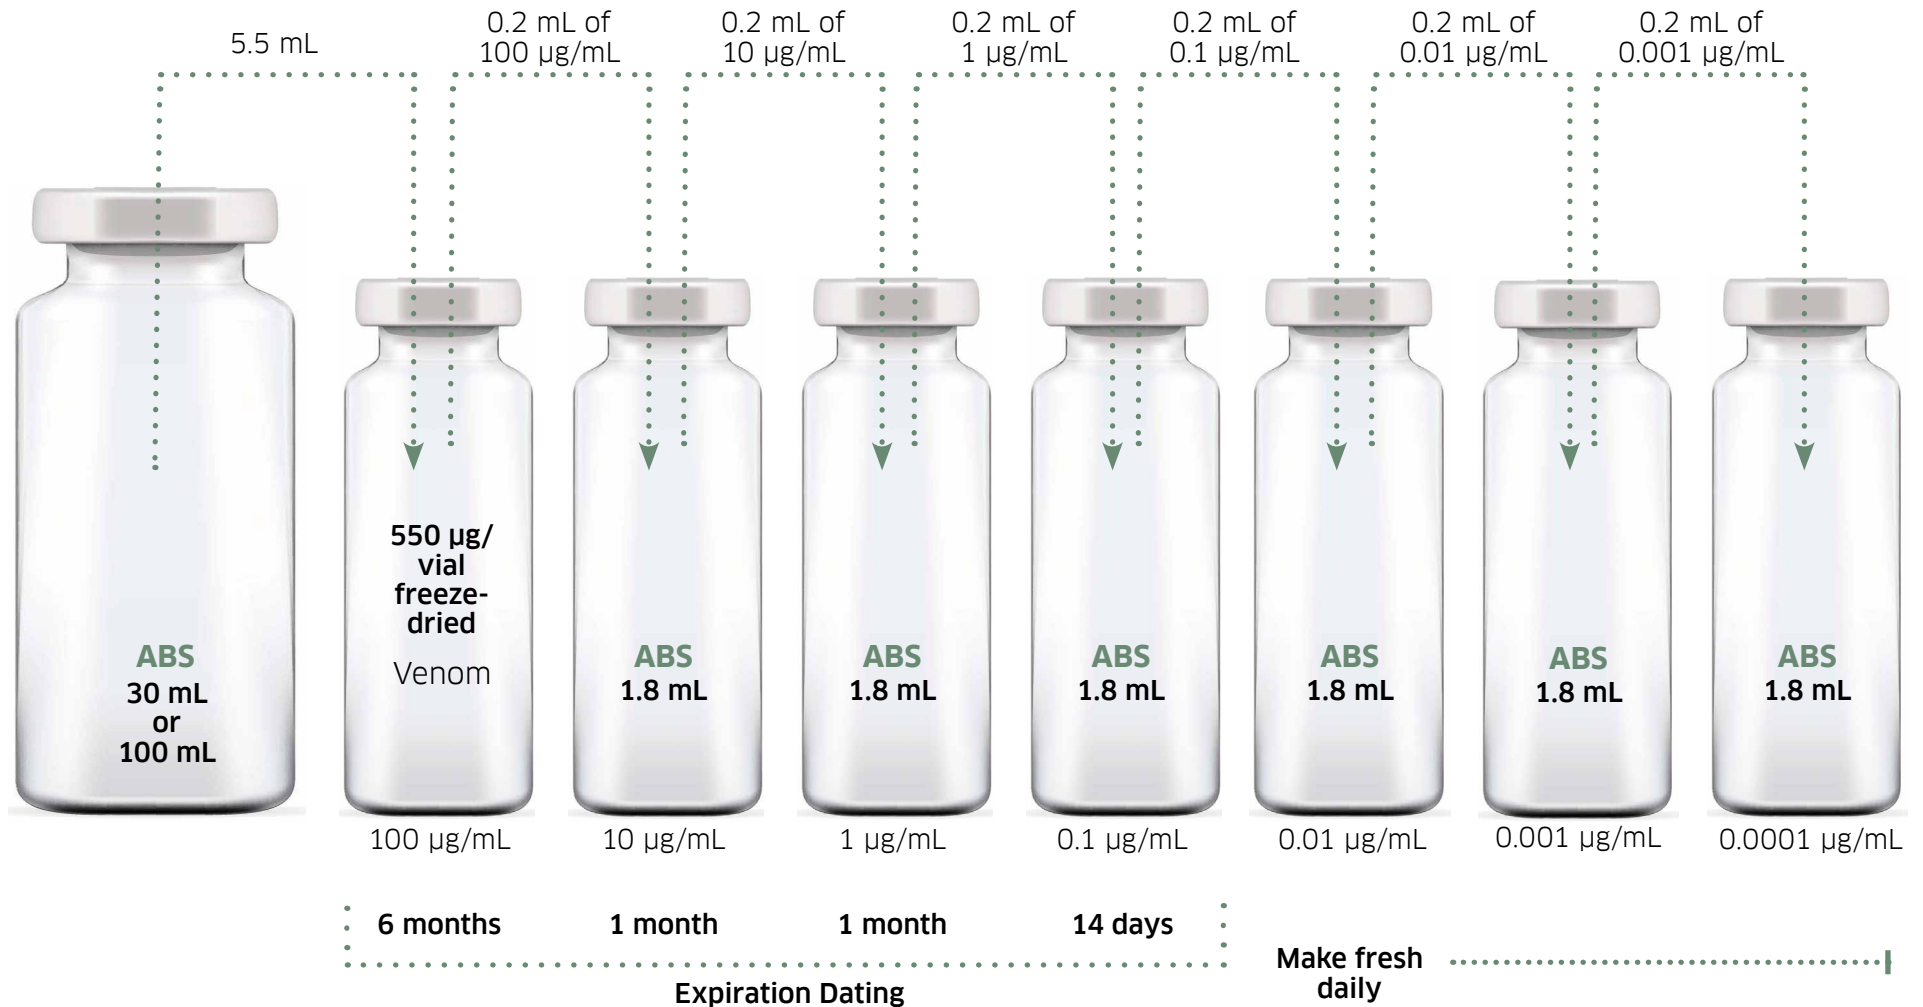

Vials not actual size. For use with HollisterStier Allergy venom products only. Always consult package insert for mixing instructions. 1 µg/mL is the recommended starting dose for scratch, prick or puncture testing. If the patient test is positive, the recommended starting doses for intradermal testing is 0.0001 to 0.001 µg/mL. Patients with a negative test may begin intradermal testing at 0.001 µg/mL.

BEFORE MIXING: Fill 2 mL sterile empty vials with 1.8 mL diluent.

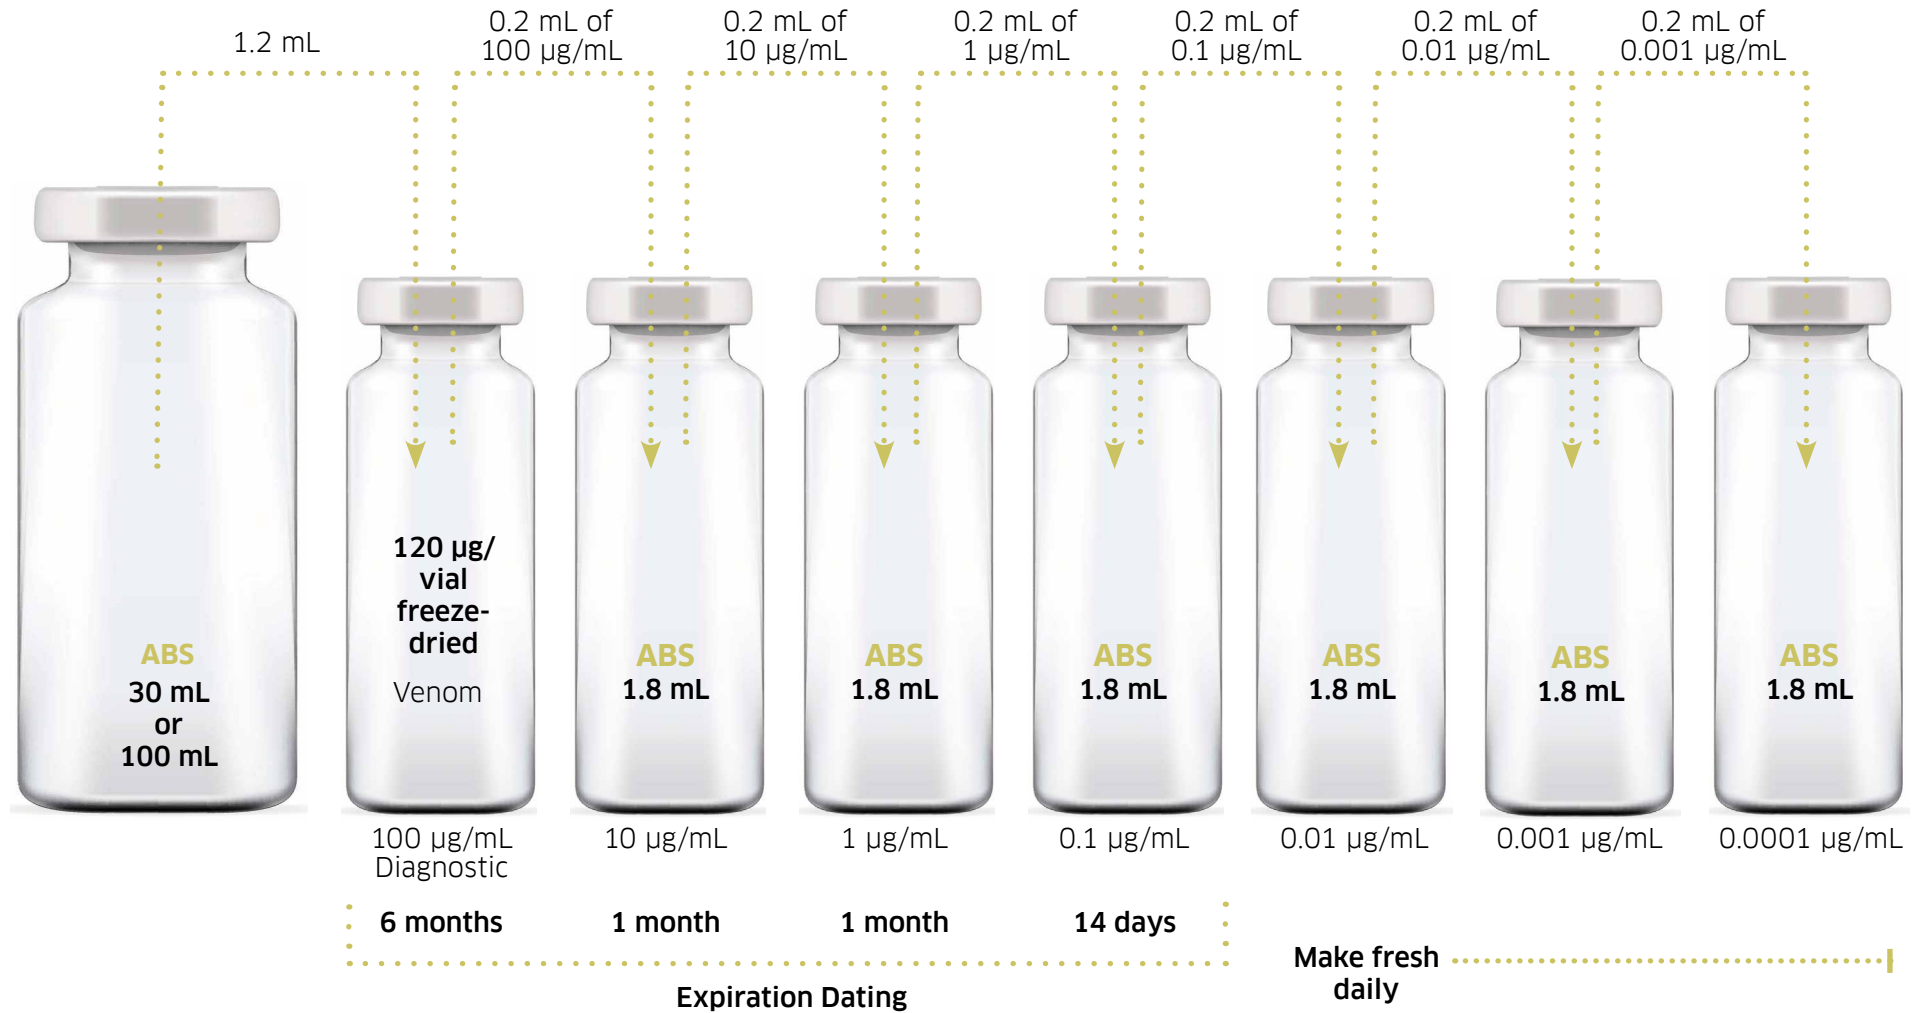

Vials not actual size.
For use with HollisterStier Allergy venom products only.
Always consult package insert for mixing instructions.